

FIG. 2A

PRIOR ART

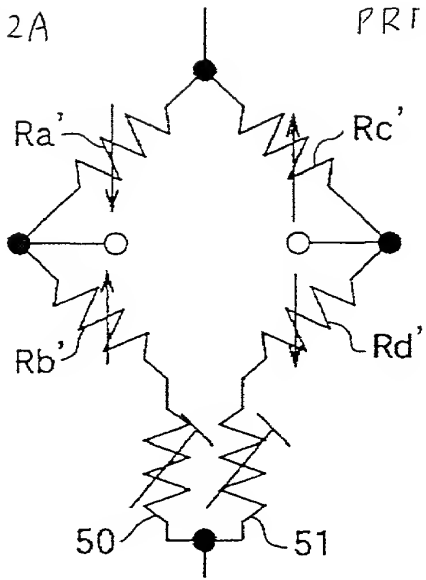
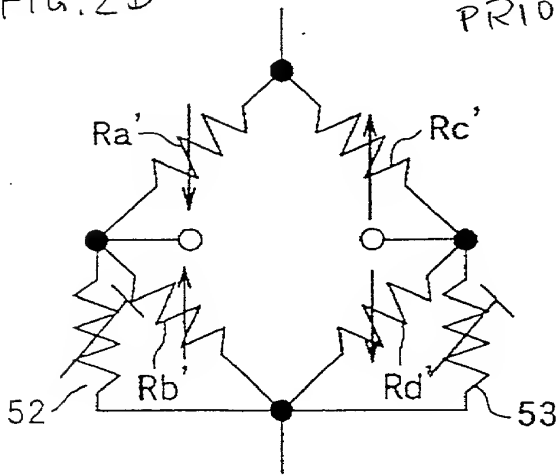


FIG. 2B

PRIOR ART







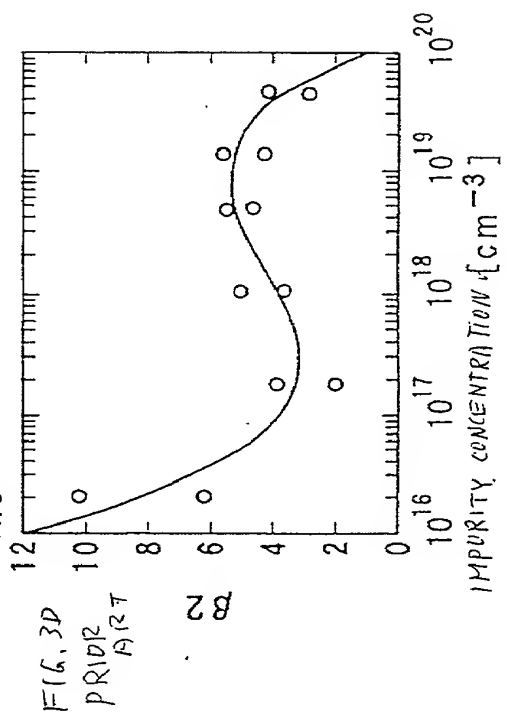


FIG. 4A

TEMP CHARACTERISTIC

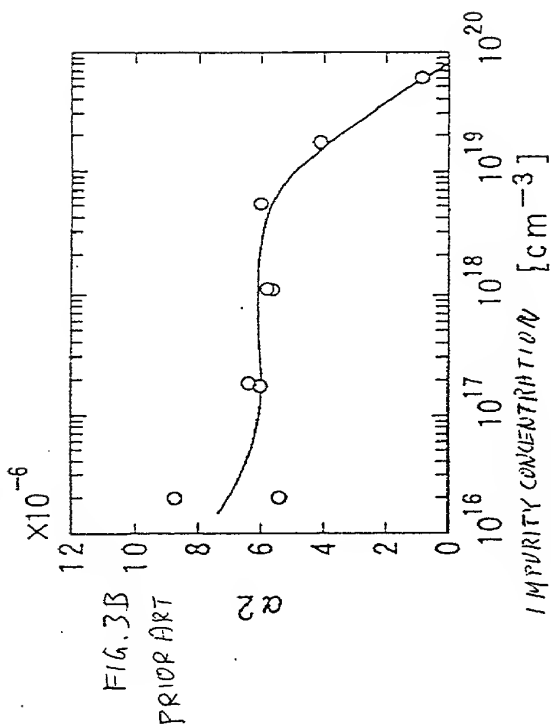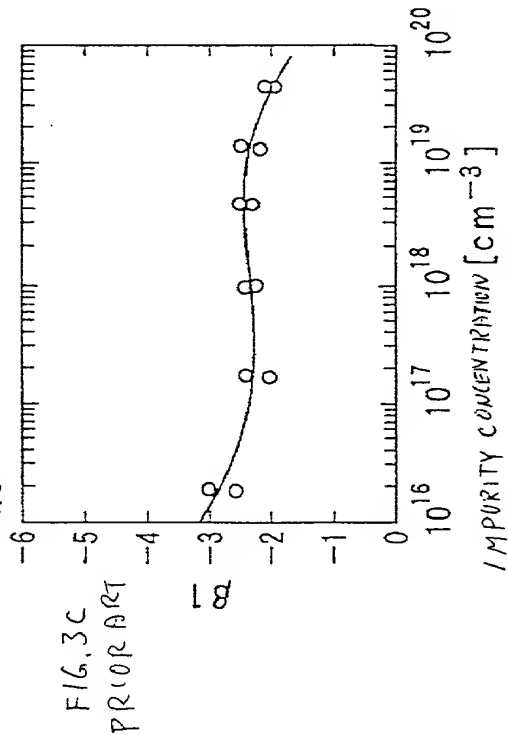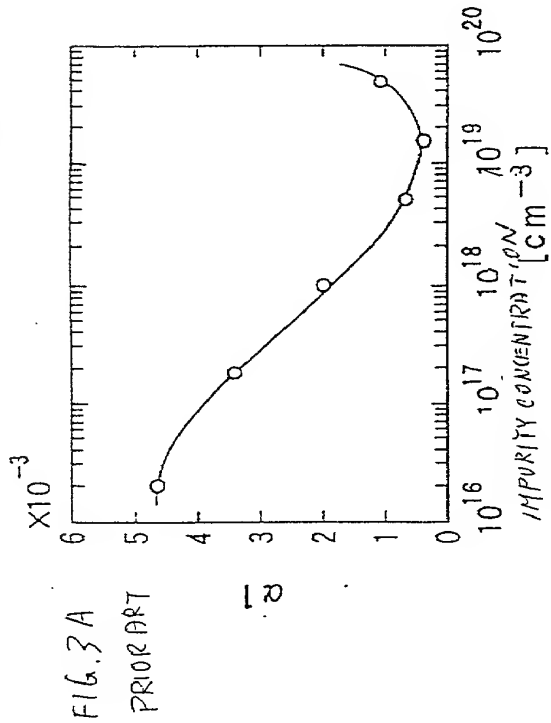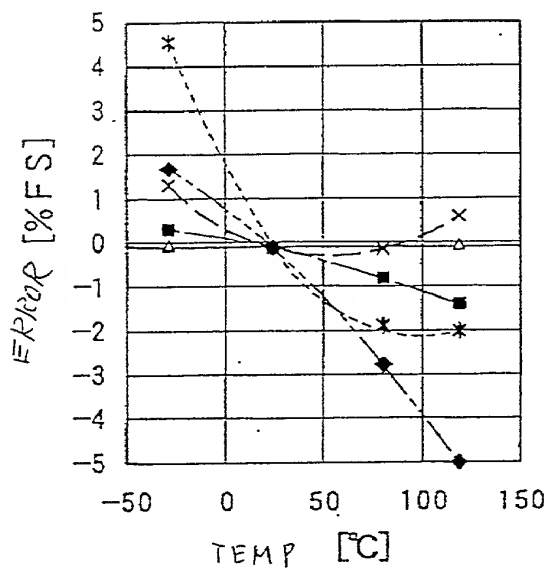


CONCENTRATION  
OF IMPURITY [ $\text{cm}^{-3}$ ]

- ◆ 4.00E+18
- 8.00E+18
- △ 1.17E+19
- × 4.00E+19
- \* 8.00E+19

FIG. 4B

TEMP CHARACTERISTIC

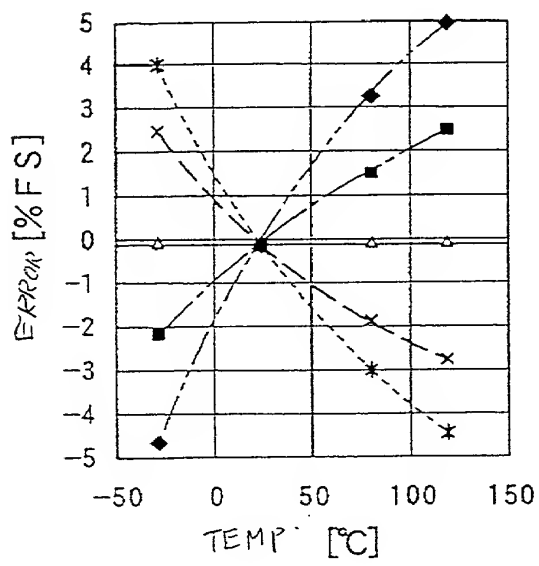

CONCENTRATION  
OF  
IMPURITY [ $\text{cm}^{-3}$ ]

- ◆ 1.60E+17
- 2.50E+17
- △ 3.64E+17
- × 5.50E+17
- \* 7.00E+17

090633-110801  
F08011-110801

FIGURE 1


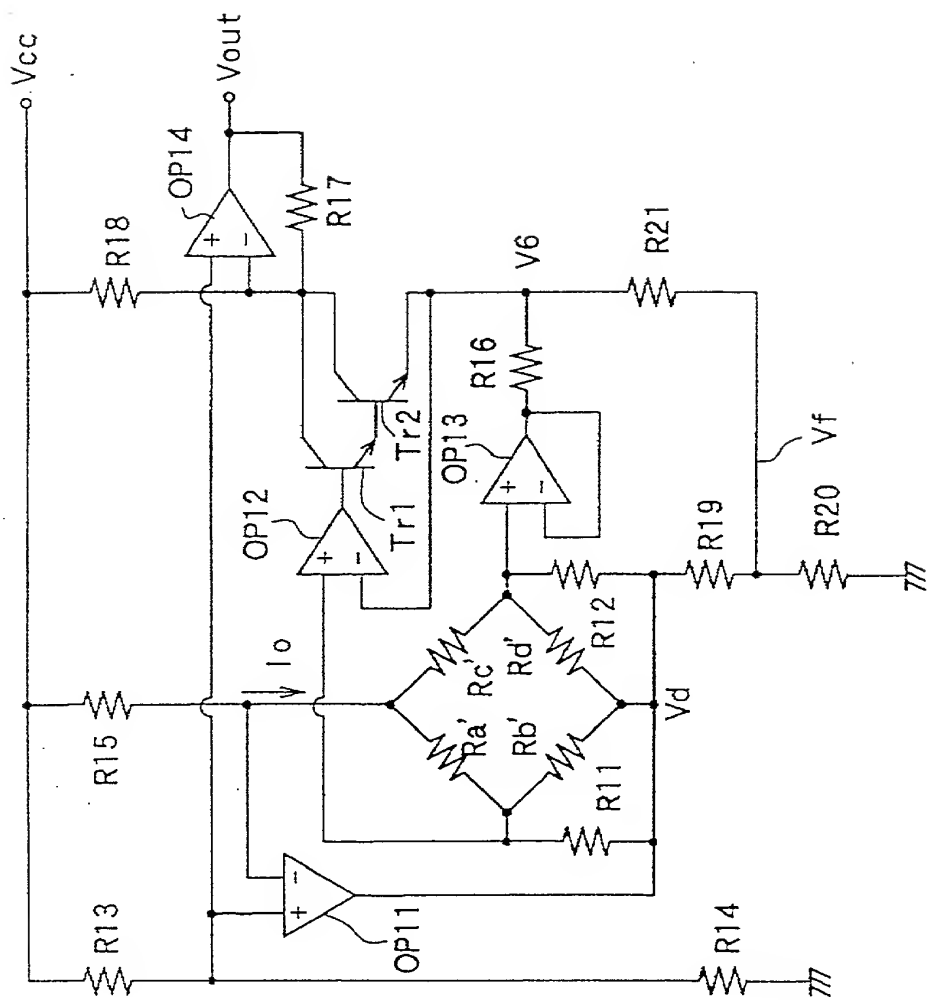


Fig. 6 Test for OP21

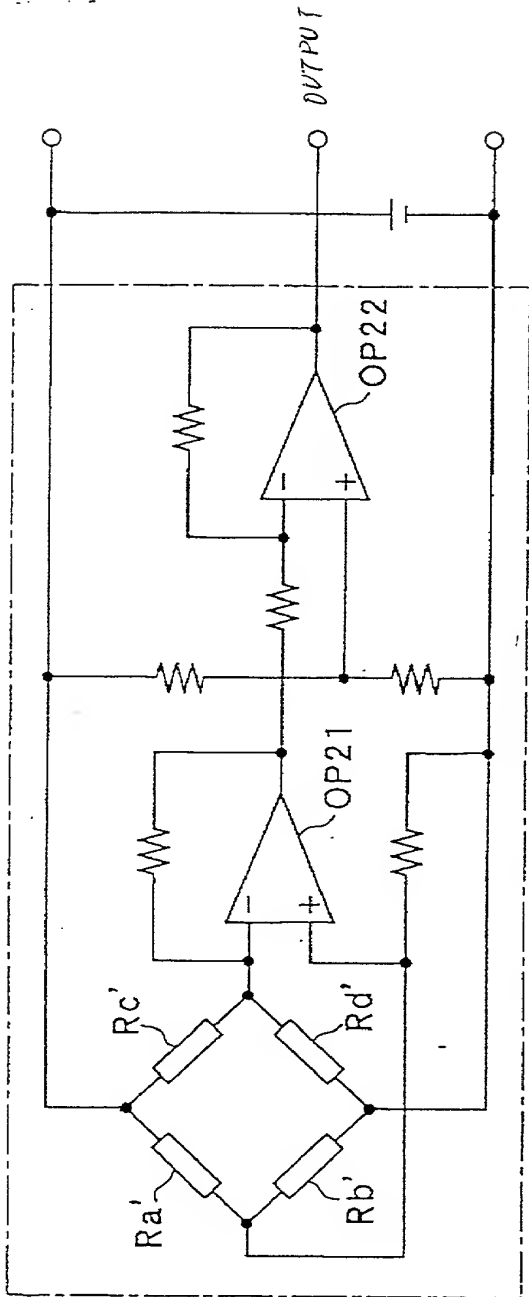

7/11

FIG. 7

PRIOR ART



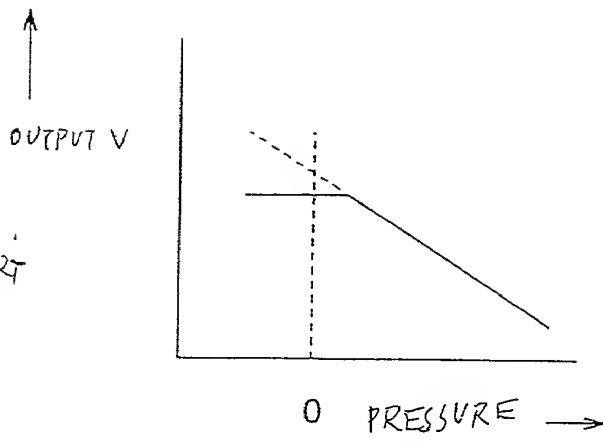


FIG. 12

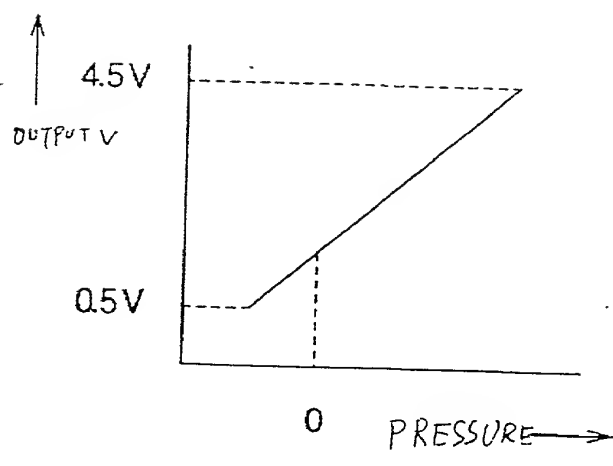

09986313.110801

FIG. 8  
PRIORITY

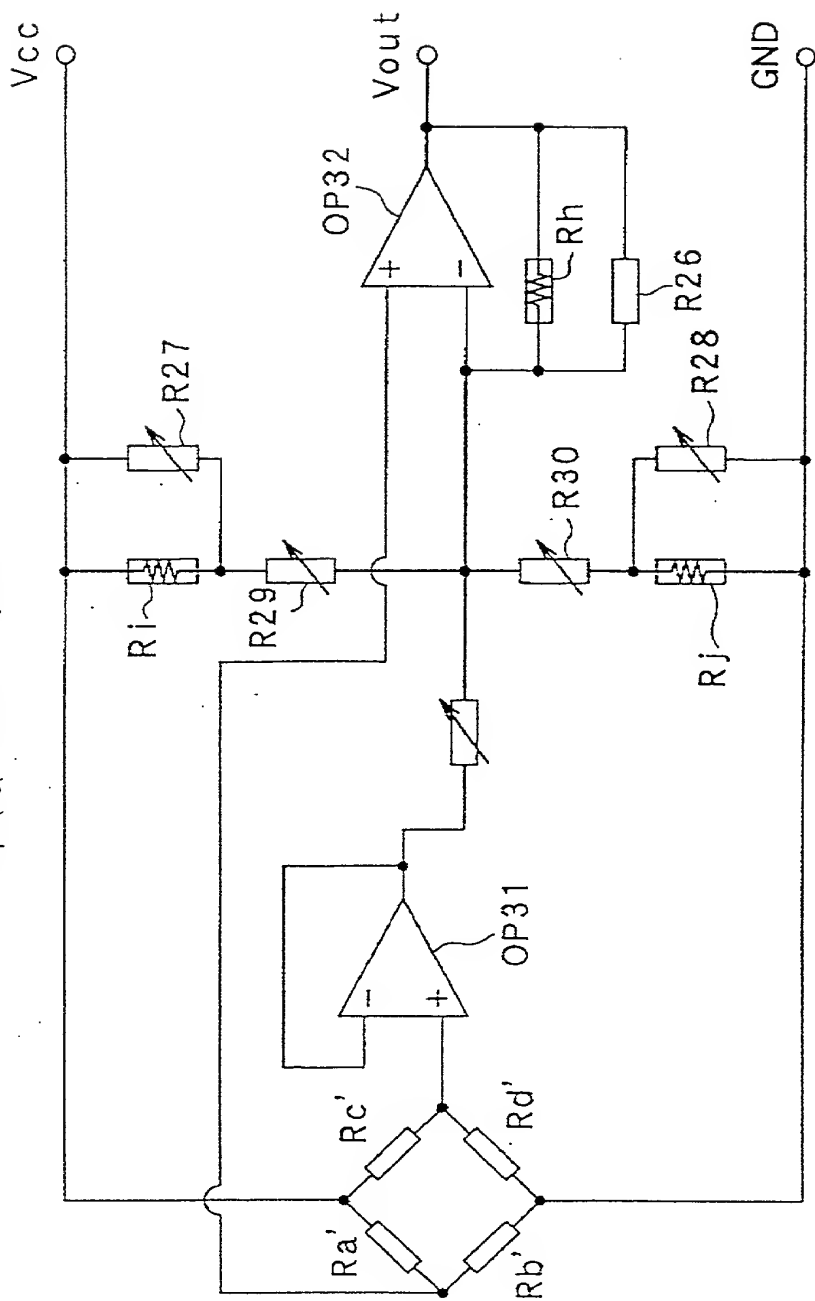



9/11

FIG. 9A


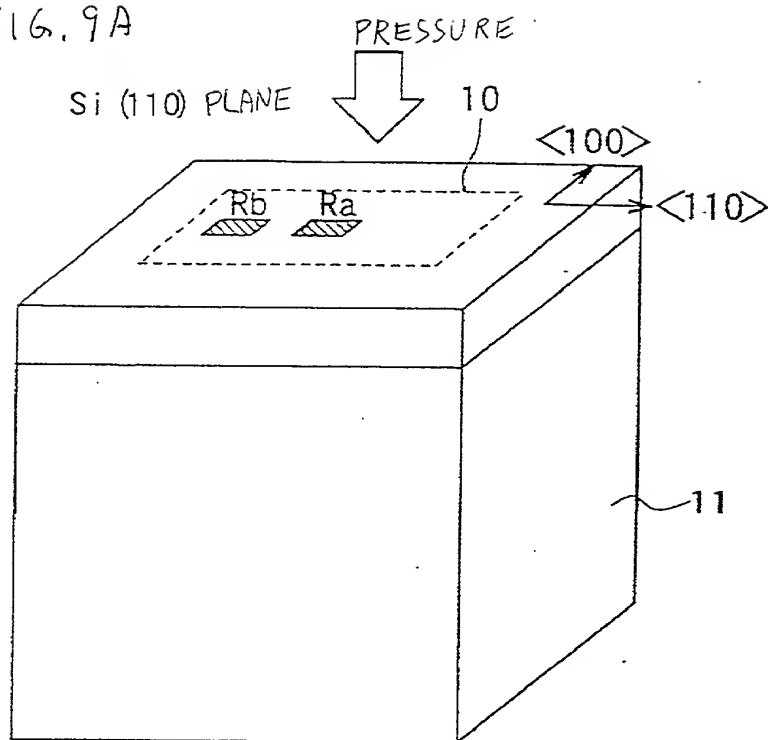


FIG. 9B



05985313.10801

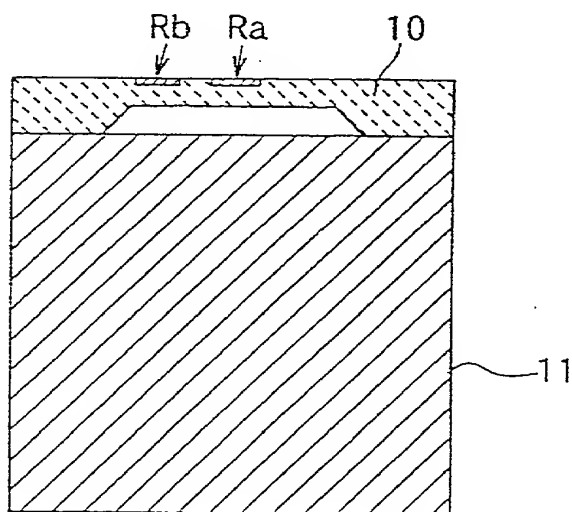